


TEST REPORT

(Electronic version)



No: 200113459

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: NMLJ-3446-44

扫码下载报告



ISSUE DATE: 2020-05-16

APPLICANT: SHENZHEN YUGUAN MEDICAL APPARATUS CO., LTD
 ADDRESS: Room 401, building C ,No2 Qiancheng Road, 228 Industrial Park ,Silian Community
 ,Henggang Street, Longgang, Shenzhen

INFORMATION CONFIRMED BY APPLICANT:

DISPOSABLE PROTECTIVE MASK (KN95)

QUANTITY: 5.1.1c

BRAND: YUGUAN

DATE RECEIVED/DATE TEST STARTED: 2020-05-09

CONCLUSION:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
FLAMMABILITY	M
HEAD BAND	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
 "—" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200113458.
 ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
 COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
 THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

5.1.2e

5.1.2e




PAGE 1 OF 4

TEST REPORT

(Electronic version)

No:200113459

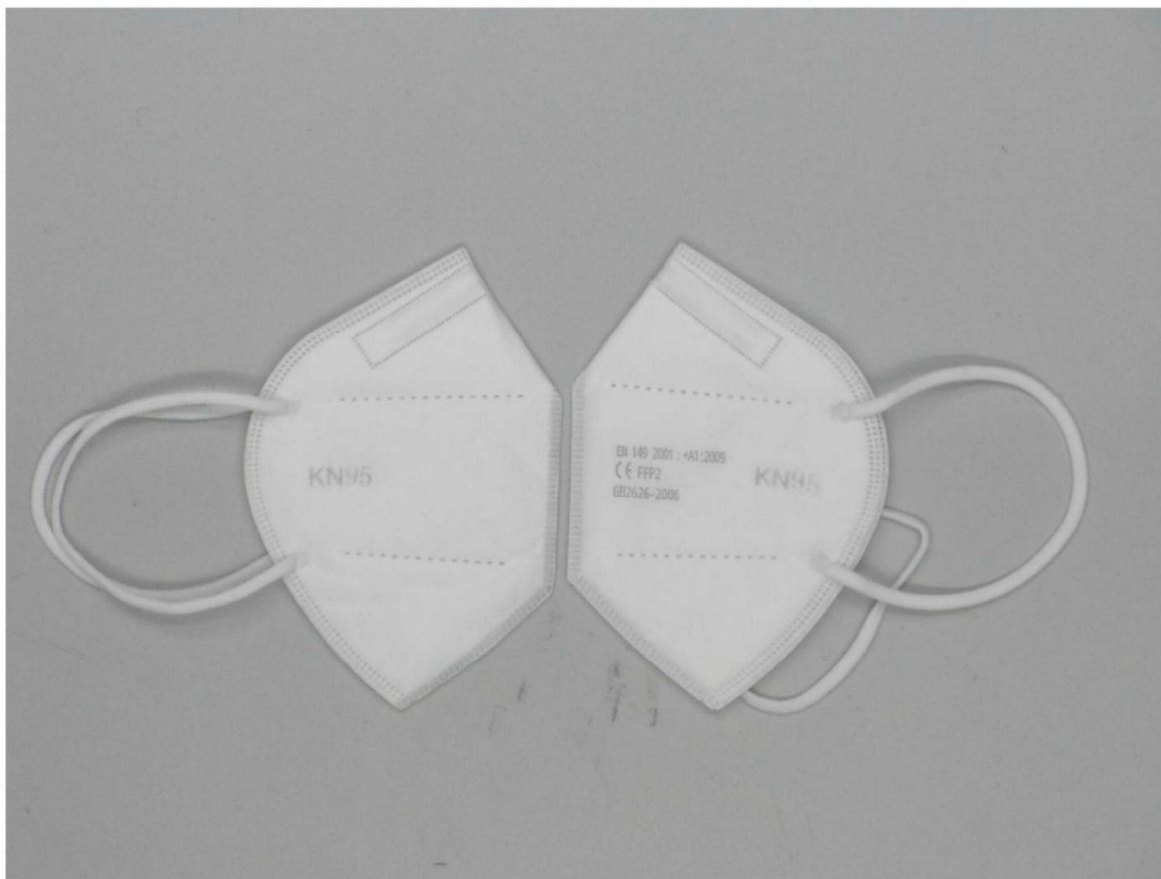

TEST REPORT

(Electronic version)

No:200113459

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER(GB 2626-2006 6.3, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION:15mg/m³, TEMP:24.1°C, RH:37.7%)**FILTRATION EFFICIENCY(%) :****UNTREATED SAMPLE**
 1# 99.254
 2# 99.315
 3# 99.189
 4# 99.360
 5# 99.327
 6# 98.96
 7# 99.312
 8# 99.254
 9# 99.220
 10# 99.187
CONDITIONING TREATED
 1# 98.65
 2# 98.54
 3# 99.102
 4# 98.59
 5# 98.60
REQUIREMENT**FILTRATION EFFICIENCY(%) :**
 ≥95.0
 (KN95)
 (GB 2626-2006)
INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:
 1# 120.1
 2# 115.4
PRETREATMENT SAMPLE:
 1# 116.7
 2# 109.8
REQUIREMENT
 ≤350
 (GB 2626-2006)
EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:
 1# 93.5
 2# 98.7
PRETREATMENT SAMPLE:
 1# 95.0
 2# 92.3
REQUIREMENT
 ≤250
 (GB 2626-2006)
FLAMMABILITY (s)

(GB 2626-2006 6.15)

AFTERFLAME TIME**UNTREATED SAMPLE**
 1# 0.0
 2# 0.0
CONDITIONING TREATED
 3# 0.0
 4# 0.0
REQUIREMENT
 AFTERFLAME TIME
 ≤5
 (GB 2626-2006)


PAGE 3 OF 4

TEST REPORT

(Electronic version)

No:200113459

HEAD BAND

(GB 2626-2006 6.11)

UNTREATED SAMPLE:

1# PASS

CONDITIONING TREATED:

1# PASS

REQUIREMENT

EACH HEAD BAND, BUCKLE AND OTHER ADJUST

PARTS OF MASK SHOULD NOT SLIP OR BREAK

UNDER 10N TENSION FOR 10S.

(GB 2626-2006)



—End of Report—

PAGE 4 OF 4