



Test Report

Report No.: GZES200301319101

Date: 2020-05-07

The following sample(s) was/were submitted and identified on behalf of the applicant as:

Applicant: XIANTAO YONGLI MEDICAL PRODUCTS CO. LTD.
 NO. 8 XIANHAN ROAD, XIANTAO, CHINA

Manufacturer: The same as the applicant

Sample Name: SURGICAL FACE MASK

Lot No. : /

Quantity: /

Model/Type Reference: YLEN104

Date of Sample Received: 2020-03-31

Date of Testing: 2020-03-31 to 2020-04-30

The Standards: EN 14683:2019

Test Items: Bacterial filtration efficiency, Differential pressure, Splash resistance pressure and Microbial cleanliness as required by the applicant

Test Result: -Please refer to next page(s)-

Remark: The test was carried out by external laboratory which assessed as competent.

5.1.2e



SGS-CSTC Standards Technical Services Co., Ltd. Guangzhou Branch



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
 Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: 5.1.2e@sgs.com
 SGS-CSTC Standards Technical Services Co., Ltd. No. 198 Kezhu Road, Science Park, Guangzhou Economic & Technology Development District, Guangzhou, China 510663 t (86-20) 82155555 f (86-20) 82075058 www.sgs.com.cn
 中国·广州·经济技术开发区科学城科珠路198号 邮编: 510663 t (86-20) 82155555 f (86-20) 82075058 5.1.2e@sgs.com

TRF No.: EN 14683_2019_a

Member of the SGS Group (SGS SA)

Page 1 of 4


Test Report
Report No.: GZES200301319101
Date: 2020-05-07
Table 1

Test Items		Result - Remarks	Test Methods
Differential Pressure (Pa/cm ²)	1	32.1	EN 14683:2019 Annex C
	2	33.3	
	3	34.2	
	4	34.0	
	5	33.6	

Table 2

Test Items		Result - Remarks	Test Methods
Splash Resistance Pressure:16.0 kPa	1	None Seen	EN 14683:2019 ISO 22609:2004
	2	None Seen	
	3	None Seen	
	4	None Seen	
	5	None Seen	
	6	None Seen	
	7	None Seen	
	8	None Seen	
	9	None Seen	
	10	None Seen	
	11	None Seen	
	12	None Seen	
	13	None Seen	



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: 512e@sgs.com

SGS-CSI Standards Technical Services Co., Ltd. No.198 Kezhu Road, Sientech Park, Guangzhou Economic & Technology Development District, Guangzhou, China 510663 t (86-20) 82155555 f (86-20) 82075058 www.sgs.com.cn
 Guangzhou Branch of SGS-CSI EEC Laboratory 中国·广州·经济技术开发区科学城科珠路198号 邮编: 510663 t (86-20) 82155555 f (86-20) 82075058 512e@sgs.com

TRF No.: EN 14683_2019_a

Member of the SGS Group (SGS SA)

Page 2 of 4



Test Report

Report No.: GZES200301319101

Date: 2020-05-07

Table 3

Test Items		Result - Remarks	Test Methods
Bacterial Filtration Efficiency (BFE)(%) Staphylococcus aureus ATCC 6538	1	> 99.9	EN 14683:2019 Annex B
	2	> 99.9	
	3	> 99.9	
	4	> 99.9	
	5	> 99.9	

Note: Control average: 2154 CFU.

Note: Mean particle size: 3.1 µm.

Note: Testing side: outside of specimen.

Note: Testing area: 39.5 cm².

Table 4

Test Items		Result - Remarks	Test Methods
Microbial Cleanliness (cfu/g)	1	5.6	EN 14683:2019 EN ISO 11737-1:2018
	2	5.9	
	3	4.6	
	4	5.7	
	5	3.4	



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: 512e@sgs.com
SGS-CS Standards Technical Services Co., Ltd. No. 198 Kezhu Road, Sientech Park, Guangzhou Economic & Technology Development District, Guangzhou, China 510663 t (86-20) 82155555 f (86-20) 82075058 www.sgs.com.cn
Guangzhou Branch of SGS SA SCS Laboratory 中国·广州·经济技术开发区科学城科珠路198号 邮编: 510663 t (86-20) 82155555 f (86-20) 82075058 512e@sgs.com

TRF No.: EN 14683_2019_a

Member of the SGS Group (SGS SA)

Page 3 of 4




Test Report

Report No.: GZES200301319101

Date: 2020-05-07

Photo documentation:

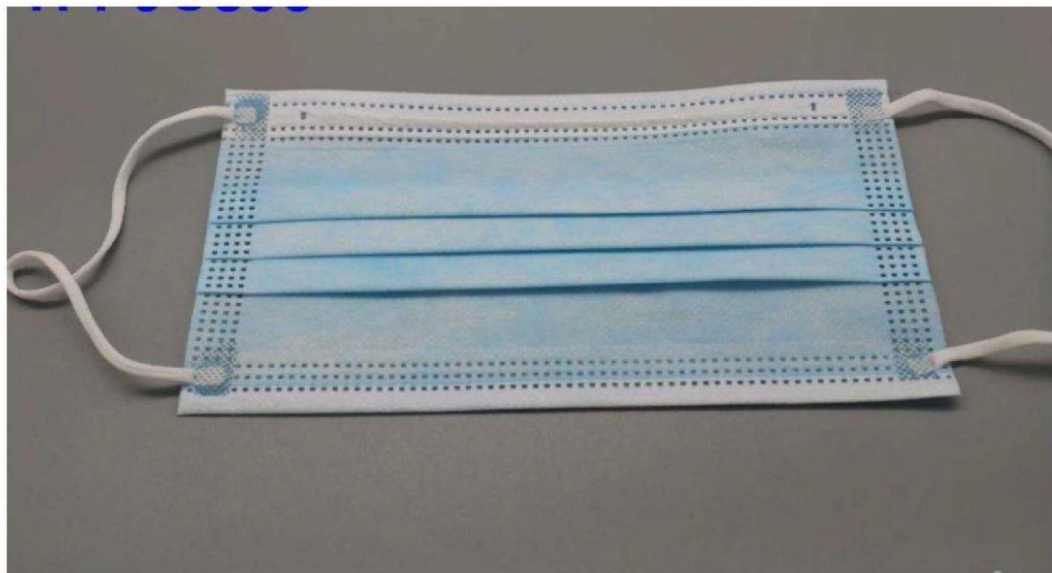

Sample description

SURGICAL FACE MASK

-- End of this report--



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: 512e@sgs.com

SGS-CSI Standards Technical Services Co., Ltd.
 Guangzhou Branch, CMAA Series 12, CMAA Laboratory

中国·广州·经济技术开发区科学城科珠路198号 邮编: 510663 t (86-20) 82155555 f (86-20) 82075058 www.sgsgroup.com.cn
 512e@sgs.com

TRF No.: EN 14683_2019_a

Member of the SGS Group (SGS SA)

Page 4 of 4