



TEST REPORT



No: 200051870

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: ULL0-8503-34

扫码下载报告



ISSUE DATE: 2020-04-01

APPLICANT: GUANGZHOU KANGLING MEDICAL SUPPLIES LIMITED
ADDRESS: _____

SAMPLE INFORMATION:

SIXTY KN95 PROTECTIVE FACE MASKS

MANUFACTURE'S NAME: GUANGZHOU KANGLING MEDICAL SUPPLIES LIMITED

DATE RECEIVED/DATE TEST STARTED: 2020-03-27

CONCLUSION:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
FLAMMABILITY	M
HEAD BAND	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"___" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200048314.
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.



APPROVED BY:

5.1.2e


5.1.2e

PAGE 1 OF 4



TEST REPORT

No:200051870

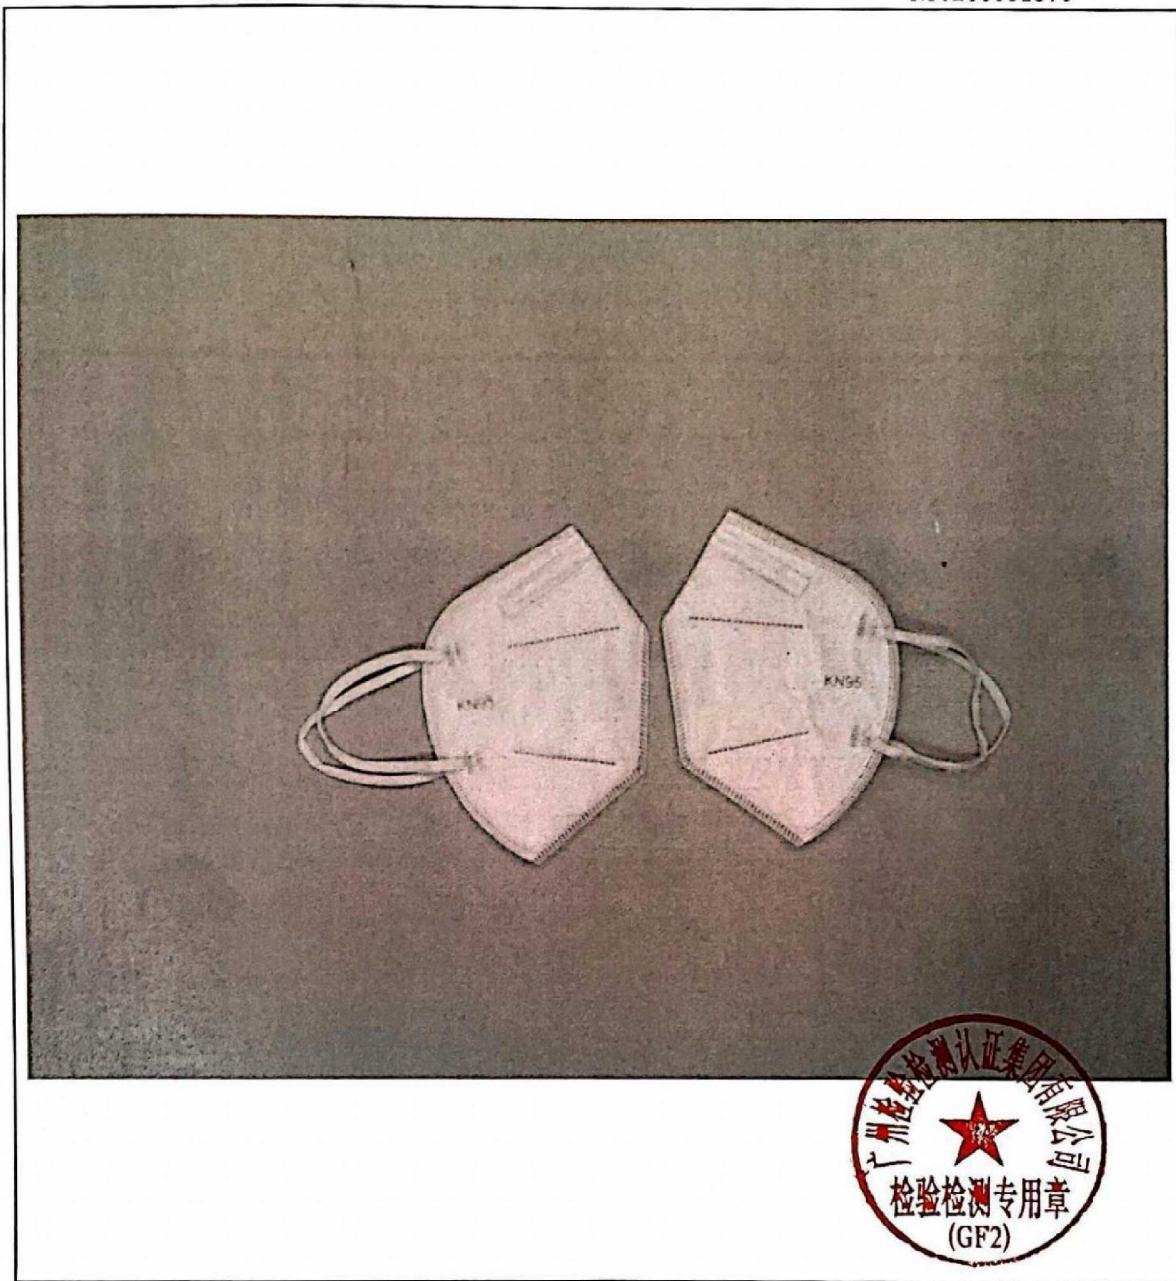

PAGE 2 OF 4



TEST REPORT

No:200051870

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER

(GB 2626-2006 6.3, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION:15mg/m³,
TEMP:23.0°C, RH:36.2%)

FILTRATION EFFICIENCY (%) :

UNTREATED SAMPLE

1# 96.70
2# 97.03
3# 96.88
4# 96.72
5# 96.54
6# 96.58
7# 96.49
8# 97.15
9# 96.94
10# 97.07

CONDITIONING TREATED

1# 95.96
2# 96.21
3# 95.75
4# 95.90
5# 96.14

REQUIREMENT

FILTRATION EFFICIENCY (%) :

≥95.0
(KN95)
(GB 2626-2006)

INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 83.1
2# 84.0

PRETREATMENT SAMPLE:

1# 121.8
2# 115.5

REQUIREMENT

≤350
(GB 2626-2006)

EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 81.0
2# 83.4

PRETREATMENT SAMPLE:

1# 96.8
2# 93.2

REQUIREMENT

≤250
(GB 2626-2006)

FLAMMABILITY (s)

(GB 2626-2006 6.15)

AFTERFLAME TIME

UNTREATED SAMPLE

1# 0.0
2# 0.0

CONDITIONING TREATED

3# 0.0
4# 0.0

REQUIREMENT

AFTERFLAME TIME

≤5
(GB 2626-2006)



PAGE 3 OF 4



TEST REPORT

No: 200051870

HEAD BAND

(GB 2626-2006 6.11)

UNTREATED SAMPLE:

1# PASS

CONDITIONING TREATED:

1# PASS

REQUIREMENT

EACH HEAD BAND, BUCKLE AND OTHER ADJUST PARTS OF MASK SHOULD NOT SLIP OR BREAK UNDER 10N TENSION FOR 10S.
(GB 2626-2006)



—End of Report—

PAGE 4 OF 4

注意事项

1. 报告书未加盖检测单位检验检测专用章无效。
2. 复印件未加盖检测单位报告确认章无效。
3. 对委托送检结果有异议的,应于报告书送达之日起十五日内提出。
4. 检测结果仅对所检样品有效。
5. 未取得资质认定的项目,仅作为科研、教学或内部质量控制之用。
6. 报告书涂改无效。

NOTE

1. The report is invalid without authorized stamp.
2. Copies of this report are invalid without authorized stamp.
3. Any dispute should be raised within 15 days after receiving the report.
4. The result is only valid for the tested sample.
5. The results of unapproved items are for reference only.
6. This report is invalid if altered.

总部:

广州市番禺区珠江路1号
电话:020-61994598 61994599
网址:<http://www.gttc.net.cn>

Headquarters:

Add: No.1, Zhujiang Road, Panyu District, Guangzhou,
Guangdong, P.R.China.
Tel: +86-20-61994598 61994599
Web:<http://www.gttc.net.cn>

花都实验室:

广州市花都区狮岭镇旗岭河滨西路1号
电话:020-37721161

Huadu Laboratory:

Add: No.1 Hebin West Road, Qiling, Huadu District, Guangzhou,
Guangdong, P.R.China.
Tel: +86-20-37721161

中大工作站:

广州市海珠区瑞康路389号长江轻纺城(新长江)南区3层
SC044号
电话:020-89637467

Zhongda Office:

Add: Room SC044, 3/F Southern Area, Changjiang (China) Fabrics & Accessories
Center, No.389 Ruikang Road, Haizhu District, Guangzhou,
Guangdong, P.R.China.
Tel: +86-20-89637467

白马工作站:

广州市越秀区站南路16号白马大厦负一层招商中心旁
电话:020-86663865

Baima Office:

Add: -1/F, Baima Building, No.16 Zhannan Road, Yuexiu District, Guangzhou,
Guangdong, P.R.China.
Tel: +86-20-86663865

西安分公司:

西安市碑林区南关正街88号长安国际中心1201室
电话:029-85213931

Xian Branch:

Add: F1201 Chang'an Metropolis Center, 88 Nanguan Street, Beilin District,
Xian, P.R.China.
Tel: +86-29-85213931